# **DATA SHEET**

### Mass Flow Controllers & Meters



# **Quantim<sup>®</sup> Series**

Low Flow Coriolis Mass Flow Meters & Controllers for Liquids & Gases

Model QmB IP40

Brooks Instrument's Quantim® Series is the smallest, lowest flow Coriolis meter and controller available on the market. With a footprint the size of a handheld organizer, you can fit this instrument into any tight space. The heart of the device is a patented Coriolis sensor design which measures low flows independent of the fluid type or process variables. With a range of 0.001 to more than 27 kg/hr, you can measure mass or volume flow and density or temperature all in one compact package. Quantim offers unsurpassed accuracy and unmatched zero stability in demanding low flow applications.

Most critical processes require control as well as measurement, and Quantim offers an optional integrally mounted, in-line control valve. No remote electronics are required as all the transmitting and control electronics are contained within the product housing. A remote valve configuration is also available.

Available with a variety of options and global approvals the Brooks Quantim Coriolis mass flow meters and controllers provide unsurpassed performance, solving specific challenges in demanding low-flow applications.

The Quantim family of Coriolis mass flow meters and flow controllers uses a proven mass flow measurement technology to provide direct mass flow measurement and control of liquids and gases that has been employed in a wide variety of markets and applications for more than 15 years. Brooks Quantim products are the smallest and lowest flow Coriolis mass flow meters and controllers available on the market. Coriolis mass flow devices have the option of using an integrally mounted or remote control valve in a miniaturized configuration. They can simultaneously measure mass or volumetric flow and fluid density or temperature.

View Quantim Series Product Page



### **Precision for Even the Most Delicate or Lowest-Flow Processes**

Quantim's Coriolis technology allows for precise, direct mass measurements even for very low flow processes. This technology enables for measurement accuracies within 0.2% of the rate for stainless steel construction and 0.5% of the rate for Alloy C-22 construction. Quantim is the lowest coriolis flow controller available. The configuration with the lowest flow capability allows for measurement down to 0.001kg/hr, which is perfect for extremely sensitive processes and costly components in any setting.

### **Process Flexibility**

The Coriolis Effect is the deflection of moving objects with respect to a reference point, utilizing this effect allows measurement of flow while negating the need for calibration to a specific fluid or process conditions. The Coriolis technology gives Quantim its' industry-leading accuracy, and allows the direct measurement of mass flow. This allows Quantim to transition between process fluids without the need for recalibration, assuming the fluid change doesn't fall out of specification for the valve assembly.

### **Material Selection for Any Application**


Quantim has material options to allow the best possible match for your needs. Quantim offers both stainless steel and Hastelloy as materials for sensor construction. This accommodates for processes with more corrosive fluids, and reduces maintenance due to corrosion of the mass flow meter/controller. Even more variety can be found in seal choices. Customers have the choice of using Viton® fluoroelastomer, Buna, Kalrez®, EPDM, and Nickel as their seals.


### **Enclosures to Meet Any Need**


Different enclosure types enable equipment to be installed in any environment from an indoor non-hazardous area to an outdoor explosion risk area. Quantim is available in four different enclosure types. The IP40 is a basic enclosure, desired for most enclosed environments. IP66 is weather/waterproof, as well as Class 1, Division 2, Zone 2 certified for hazardous locations. The IP66XP is Division 1, Zone 1 certified for explosive environments. No matter the environment, Quantim can be tailored to fit your needs.


### **Features and Benefits**


| Features   | Benefits   |
|--|--|
| Integrated sensor, valve and PID control all in one small package      | Simplifies purchase, installation, and start up by having everything available from one supplier in a single compact unit  |
| Low mass tube drive and optical sensing                                | Enables accuracy at extreme low flow   |
| Multivariable outputs and true mass measurement                        | Improves and simplifies process monitoring and diagnostics, further reducing cost of ownership   |
| Diagnostic alarms and warnings   | Provides early indication of potential process issues so preventative actions can be taken   |
| Industry leading mass flow measurement precision                       | Process chemistry and/or process conditions can be altered without the need to change or recalibrate the measurement system, providing the user with maximum flexibility |
| No internal moving parts   | Minimizes maintenance requirements and overall cost of ownership   |
| Small physical size  | Easily integrated into most intricate process systems  |
| Gas and liquid measurement and control capability in one package       | The ultimate in process flexibilty   |
| Variety of options, enclosure types and area classifications available | The right product for your application   |

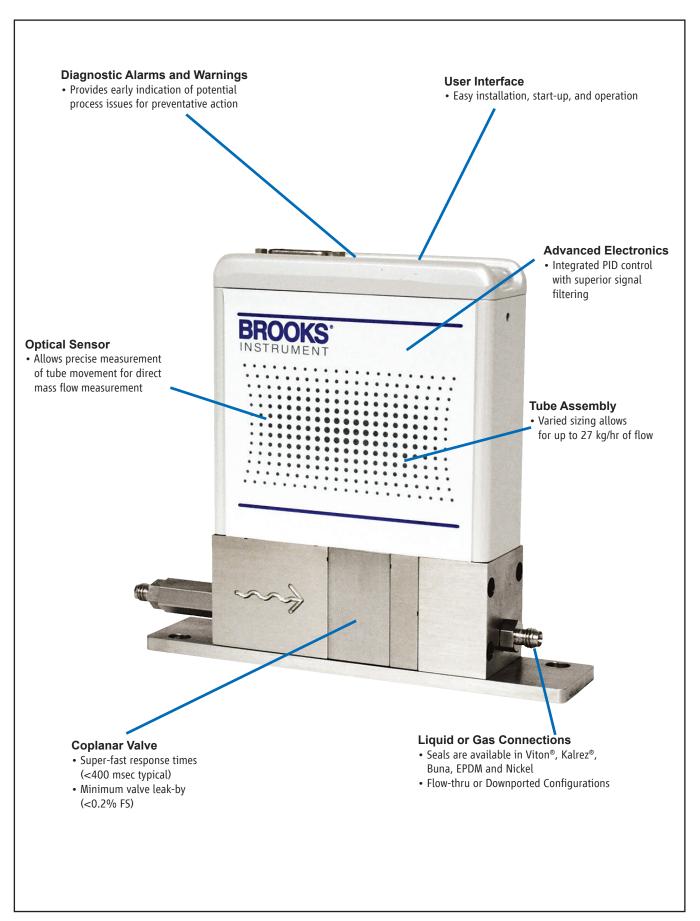

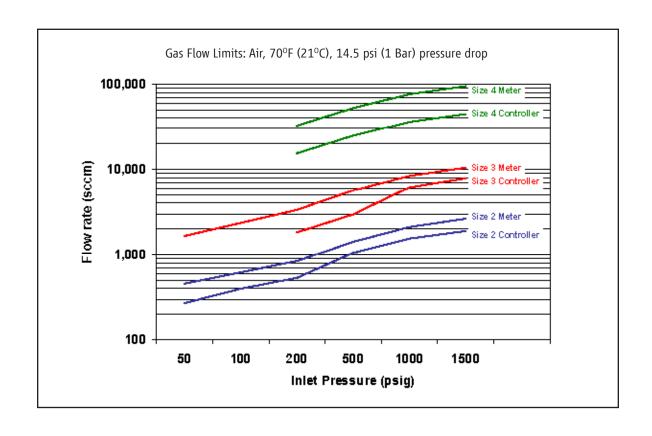

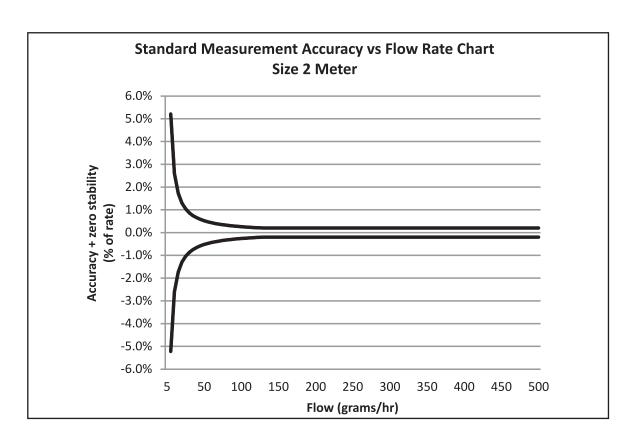

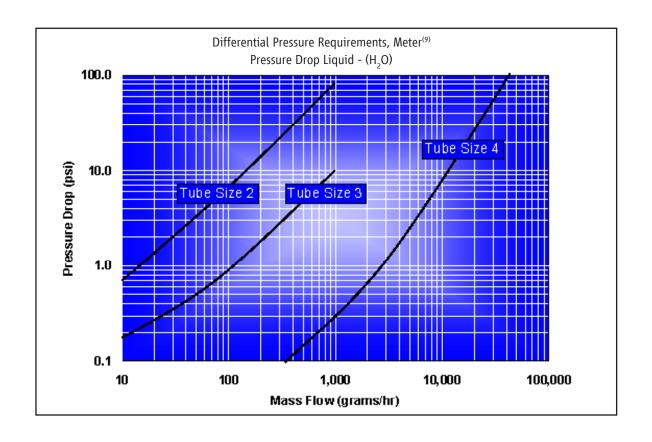

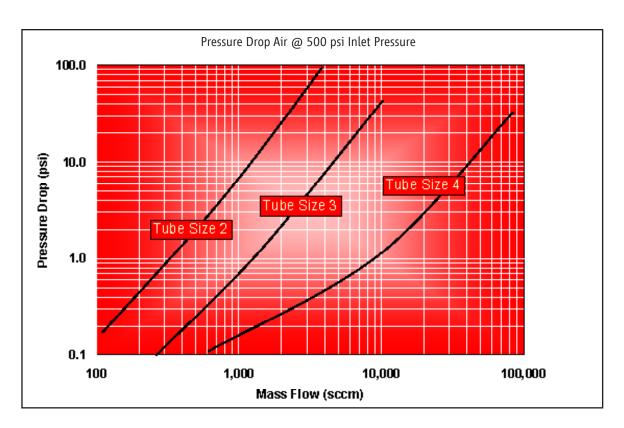

# **Product Specifications**

|  |  | 01105/5  |  |                |                        | OMPH (III )                  |                |  |  |  |
|--|--|--|--|----------------|------------------------|------------------------------|----------------|--|--|--|
| DEDECORMANICE  | _  | QMBC (Controlle                                | r)                                     |                |                        | QMBM (Meter)                 |                |  |  |  |
| PERFORMANCE  | 2  | 2  |  |                | 2                      | 2                            |                |  |  |  |
| Tube Size: Nominal Flow Range: Liquid (kg/hr) <sup>(5)</sup> :     | 0.15   | 3<br>0.78                                      | 4<br>7.97                              |                | 0.19                   | 1.00                         | 4<br>13.50     |  |  |  |
| Gas (kg/hr):   | 0.076  | 0.214  | 1.796                                  |                | 0.103                  | 0.405                        | 3.840          |  |  |  |
| Gas (sccm) <sup>(2)</sup> : Minimum Measurable Flow Liquid (kg/hr) | 1051<br>0.001  | 2955<br>0.010                                  | 24787<br>0.100                         |                | 1432<br>0.001          | 5595<br>0.010                | 53116<br>0.100 |  |  |  |
|  | 0.001  |  | 0.100                                  |                | 0.001                  |                              |                |  |  |  |
| Zero Stability:<br>Stainless Steel Sensor (kg/hr):                 | 0.00026  | QMBC (Controller)<br>0.0020                    | 0.0120                                 |                | 0.00026                | QMBM (Meter<br>0.0020        | o.0120         |  |  |  |
| Alloy C-22 Sensor (kg/hr):   | 0.0004   | 0.0030   | 0.0240                                 |                | 0.0004                 | 0.0030                       | 0.0240         |  |  |  |
| Repeatability & Reproducibility:                                   | $\pm 0.05\%$ or $\pm [0.5$ x (zero stability/flowrate) x 100]% of rate whichever is greater  |  |  |                |                        |                              |                |  |  |  |
| Response Time (Settling Time):                                     |  |  |  |                |                        |                              |                |  |  |  |
| 2% F.S. of final value,<br>(per SEMI Guideline E17-91)             |  | tainless Steel: <2 sec<br>Alloy C-22: <12 seco |  |                |                        | <0.5 seconds<br><0.5 seconds |                |  |  |  |
| Flow Accuracy (Standard Flow):                                     |  | dard Flow Accuracy o                           |  | ow rot         | a) v 10010/2 of rato   |                              |                |  |  |  |
| Stainless Steel Sensor:  | Stain  | data Flow Accuracy o                           | Liquid: 0.2%                           |                |                        | willchever is greater        |                |  |  |  |
| Hastelloy Sensor:  |  |  | Liquid: 0.5%                           | Gas: (         | ).5% of rate           |                              |                |  |  |  |
| RATINGS  |  |  |  |                |                        |                              |                |  |  |  |
| Operating Temperature Range:                                       |  |  | 0 to                                   | 60°C           |                        |                              |                |  |  |  |
| Temperature Accuracy:  |  |  | ± 0                                    | .5°C           |                        |                              |                |  |  |  |
| Differential Pressure Range:                                       |  |  | Liquid: 10                             | to 20          | 00 nsi                 |                              |                |  |  |  |
| Sincicinal ressure nanger  |  |  | Gas: 10                                |                |                        |                              |                |  |  |  |
| Density Range:   |  |  | 0 to 0.3 and                           | 0.5 to         | 2.0 g/cc               |                              |                |  |  |  |
| Density Accuracy:  |  |  | ± 0.0                                  | 05 g/d         | C                      |                              |                |  |  |  |
| Maximum Operating Pressure:  |  |  |  |                |                        |                              |                |  |  |  |
| Standard:<br>Optional:   |  |  |  | ) psi<br>0 psi |                        |                              |                |  |  |  |
| Optional:  |  |  |  | 0 psi          |                        |                              |                |  |  |  |
| Leak Integrity (external):   |  |  |  |                | n. cc/sec., helium (m  | ax)                          |                |  |  |  |
|  |  | Meta   | al Seal: 1 x 10 <sup>-10</sup> at      | m. cc/         | sec., helium (max)     |                              |                |  |  |  |
| MECHANICAL   |  |  |  |                |                        |                              |                |  |  |  |
| Materials of Construction  |  |  |  |                |                        |                              |                |  |  |  |
| Process Wetted: Optional:  |  | 316L, 316                                      | L VAR, High alloy fo<br>Alloy C-22 s   |                | stainless and 17-7F    | 'H                           |                |  |  |  |
| Process Seals:   |  | Elastomer Sea                                  |  |                | rs, Buna, Kalrez or E  | PDM                          |                |  |  |  |
|  |  | I  | Metal Seal: stainles                   | s stee         | l and nickel           |                              |                |  |  |  |
| Housing:   |  |  | 240: polyurethane                      |                |                        |                              |                |  |  |  |
|  |  | Ir   | P66: polyurethane<br>IP66XP: al        |                |                        |                              |                |  |  |  |
| Inlet Filter:  |  | Tube size 2 contro                             | oller: 1 micron or 1                   | 0 mic          | ron inlet filter recon | nmended                      |                |  |  |  |
|  | Tube size 3 or 4: 10, 20, 30 & 40 micron filters available   |  |  |                |                        |                              |                |  |  |  |
| Weight:  |  |  | Housing IP40: 1.                       | _              |                        |                              |                |  |  |  |
|  |  |  | Housing IP66: 1. Housing IP66XP:       | _              |                        |                              |                |  |  |  |
| Moisture Content:  | , , , , , , , , , , , , , , , , , , ,  |  |  |                |                        |                              |                |  |  |  |
| modure content.  | Purged to exhaust dew point less than -40°C (-40°F) prior to shipment to remove calibration liquid, to prevent process contamination. Then vacuum bagged at ambient room conditions. |  |  |                |                        |                              |                |  |  |  |
| Process Fitting Options:   | 1/   | /16", 1/8", 1/4" or 6<br>Down                  | mm tube compress<br>port ANSI/ISA 76.0 |                |                        | 3.2 mm UPG,                  |                |  |  |  |
| Electrical Connections:  |  |  | : 15 pin D-Type con                    |                |                        |                              |                |  |  |  |
|  |  |  | Unpluggable Term                       |                |                        | connector                    |                |  |  |  |
| Discouries   |  | IP66XP: 3/4" NPT wi                            | •                                      |                | , ,,                   | e connector.                 |                |  |  |  |
| Dimensions:  |  |  | (See Figures 1                         | thro           | ıgn /)                 |                              |                |  |  |  |
| DIAGNOSTICS  |  |  |  |                |                        |                              |                |  |  |  |
| Status Lights:   |  |  | Status and                             | Alarr          | n LEDs                 |                              |                |  |  |  |
|  |  |  |  |                |                        |                              |                |  |  |  |

Electrical

**Output Signals:** 4-20 mA and 0-5 Vdc active output represents mass flow or volume flow (3)

And simultaneously available 4-20 mA or 0-5 Vdc active ouput represents on-line density or

temperature information.

Alarm output, max. voltage 30 Vdc, max. current 100 mA

Input Signals:

Command (setpoint) that drives the control valve, either 4-20 mA or 0-5 Vdc input signals

Valve Override Function:

Left floating/unconnected - instrument controls flow at setpoint Connected to signal at or above 5.0 volts - valve is forced open Connected to signal at or below 0.0 volts - valve is forced closed

Power Requirements:

**Nominal Current:** 

Maximum Current:

Maximum Power:

Voltage: +14 to 27 Vdc(12) Controller: 300 mA to 400 mA Meter: 100 mA to 150 mA Controller: 715 @ 14 Vdc Meter: 470 mA @ 14 Vdc Controller: 10.0 W

Meter: 6.6 W

Additional Functions and Outputs

Damping:

Factory set time constant from 0 to 10 seconds

LED's:

'STAT' solid green: system operative 'AL' solid red: system fault

Pushbutton:

'ZERO' setting pushbutton

Certifications, Approvals and Compliance

IP40 Series:

US and Canada

UL Recognized E73889, Vol 3, Section 3.
Non Incendive, Class I Division 2 Groups A, B, C and D; T4
per UL 1604, UL 508, and CSA 22.2 No. 213 1987; C-22.2 No. 14-M91
Ex nC IIC T4 per CSA E79-15

Europe

KEMA 04ATEX1241 X

II3G Ex nA II T4 per EN 60070-15: 2003

IP66 Series:

US and Canada UL Recognized E73889, Vol 1, Section 26 (conduit entry)

UL E73889, Vol. 3, Section 3 (cable gland entry) Non Incendive, Class I Division 2 Groups A, B, C and D; Dust Ignition-Proof, Class II, Division 2, Groups F and G; Suitable for Class III, Division 2, T4 per UL 1604, UL 508, and CSA 22.2 No. 213 1987; C-22.2 No. 14-M91

Ex nC IIC T4 per CSA E79-15

Class 1, Zone 2, AEx nC IIC T4 per ANSI/UL 60079-15

Europe

II 3 G Ex nA II T4 and II 3D T 135°C

per EN 60079-0: 2006, EN 60079-15: 2005, EN 61241-0: 2006, EN 61241-1: 2004,

IEC 60079-0: 2004, IEC 60079-15: 2005, IEC 61241-0: 2004, IEC 61241-1: 2004

Korea

KOSHA

20-AV4BO-0108X Ex nA IICT4 Ex tD A22 IP66 T85°C

**IP66XP Series:** 

US and Canada

UL Recognized E73889, Vol 1, Section 21. UL E73889, Vol. 3, Section 3 (cable gland entry)

Explosion-Proof, Class I Division 1 Groups C and D; Dust Ignition-Proof, Class I, Division 1, Groups E, F and G; Suitable for Class III, Division 1, T4 per ANSI/UL 1203 and

CSA 22.2 No. 30

Class 1 Zone 1, ex d IIB per CSA E600 79-0, CSA E60079-1 Class 1 Zone 1, AEx d IIB per UL 60079-0, UL 60079-1

Europe

II 2 G Ex d IIB T6 and II 2 D T 85°C per EN 60079-0: 2006, EN 60079-1: 2007, EN 61241-0: 2006,

EN 61241-1: 2004

**Environmental Compliance** 

EMC Directive 2014/30/EU per EN 61326-1: 2013 ROHS Directive 2011/65/EU

Pressure Effects Compliance

Pressure Equipment Directive 2014/34/EU

"Sound Engineering Practice"

#### Notes

- (1) The nominal flow rate is the flow rate at which water at reference conditions causes approximately 1 bar of pressure drop or the laminar to turbulent transition flow whichever is lower. Maximum flow rate is twice nominal flow rate or the laminar to turbulent transition flow whichever is lower.
- $^{\scriptscriptstyle{(2)}}$  Standard volumetric conditions are 14.696 psia and 70°F.
- (3) Actual volumetric flow is a function of the mass flow and the density measurements; therefore the accuracy of actual volumetric flow is a function of the mass flow and density accuracy.
- (4) Accuracy includes combined repeatability, linearity, and hysteresis. Specifications are based on reference test conditions of water/nitrogen at 68 to 77°F (20 to 25°C) and 15 to 30 psig (1 to 2 bar).
- (5) Differential pressures are based on reference conditions of water and air at 68 to 77°F (20 to 25°C).
- (6) The density measurement at temperatures other than 21°C (70°F) has an additional error of approximately 0.0005 grams/cc per °C.
- (7) A temperature rise of up to 20°C (68°F) from internal heating can occur in an open environment where ambient temperature is 23°C (73°F). The device temperature is affected by the ambient and process temperature as well as warming when the device is powered. The device should be maintained in the specified temperature range at all times.

# Product Dimensions - QmB IP40 Downported

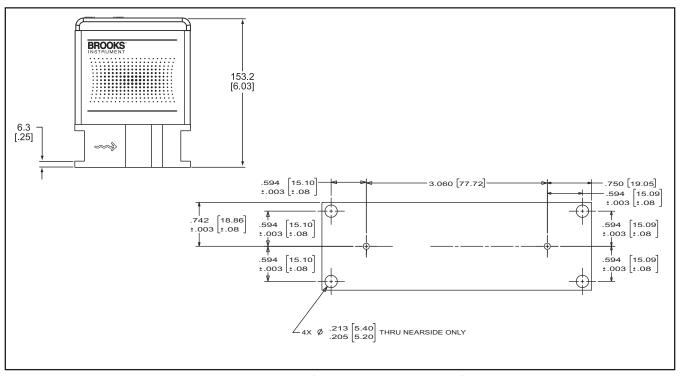


Figure 1 Dimensional Drawing QmB IP40 Downported

| Quantim Patent Numbers as follow |                           |
|----------------------------------|---------------------------|
| ArgentinaAR026329B1,             | AR021594B1                |
| Australia                        | 778137, 771345, 782183    |
| Canada                           | 2389433                   |
| China                            | ZL00817949.2, 171140      |
| Federation of Russia             | 2272257, 2263284, 2277227 |
| Germany                          | 40004270.3                |
| Hong Kong                        | HK1051720                 |
| India                            |                           |
| Indonesia                        | 3660/2006, ID0015789      |
| Japan                            |                           |

| Malaysia                          | MY-128330-A                     |
|-----------------------------------|---------------------------------|
|                                   | 242129, 244688, 231280          |
| Singapore                         | 122105, 123306, 88632, 81430    |
| South Korea                       | 678430                          |
| Switzerland                       | 127118                          |
| UK                                | 2092458                         |
| US D436876, 48438                 | 890, 4996871, 5231884, 5295084, |
| 5555190, 5687100, 59293           | 344, 6226195, 6476522, 6487507  |
| 6505131, 6505135, 65129           | 987, 6513392, 6526839, 6748813  |
| 6769                              | 9301, 7032462, 7111519, 7117751 |
| Counterparts in other countries a | nd other patents pending        |

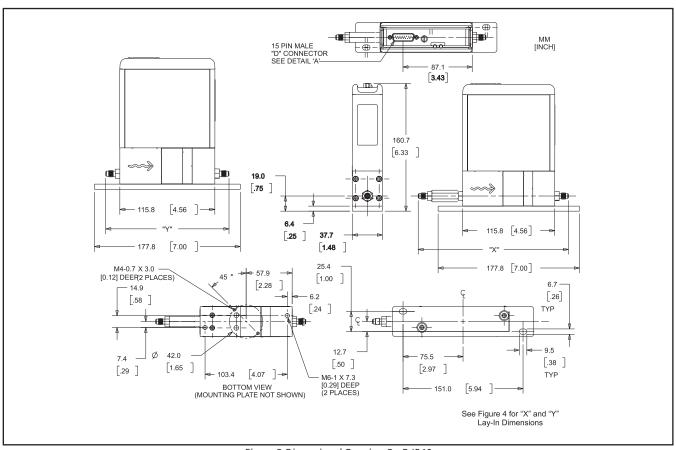


Figure 2 Dimensional Drawing QmB IP40






Figure 3 D-Connector Electrical Pin Connections

| FITTING  | "X" Dimension                   | AL VALVE<br>"Y" Dimension       | REMOTE "X" Dimension           | "Y" Dimension                  |  |  |  |
|--|---------------------------------|---------------------------------|--------------------------------|--------------------------------|--|--|--|
| 1/16" Tube<br>Compression  | 184.1 [7.25]*<br>167.3 [6.59]** | 151.9 [5.98]*<br>135.1 [5.32]** | 340.1 [13.39]<br>323.3 [12.73] | 307.9 [12.12]<br>291.1 [11.46] |  |  |  |
| 1/8" Tube<br>Compression   | 192.7 [7.59]*<br>167.3 [6.59]** | 160.5 [6.32]*<br>135.1 [5.32]** | 348.7 [13.73]<br>323.3 [12.73] | 316.5 [12.46]<br>291.1 [11.46] |  |  |  |
| 1/4" Tube<br>Compression   | 197.3 [7.77]*<br>166.8 [6.57]** | 165.1 [6.50]*<br>134.6 [5.30]** | 353.6 [13.92]<br>323.1 [12.72] | 321.4 [12.65]<br>290.9 [11.45] |  |  |  |
| 6 mm Tube<br>Compression   | 197.6 [7.78]*<br>167.0 [6.78]** | 165.4 [6.51]*<br>134.8 [5.31]** | 353.9 [13.93]<br>323.2 [12.72] | 321.7 [12.67]<br>291.0 [11.46] |  |  |  |
| 1/8" NPT (F)   | 179.9 [7.08]                    | 147.7 [5.81]                    | 335.9 [13.22]                  | 303.7 [11.96]                  |  |  |  |
| 1/4" NPT (F)   | 189.3 [7.45]                    | 157.1 [6.19]                    | 345.3 [13.59]                  | 313.1 [12.33]                  |  |  |  |
| 1/8" VCR   | 182.6 [7.19]                    | 150.4 [5.92]                    | 338.6 [13.33]                  | 306.4 [12.06]                  |  |  |  |
| 1/4" VCR   | 200.9 [7.91]                    | 168.7 [6.64]                    | 356.2 [14.02]                  | 324.0 [12.76]                  |  |  |  |
| 1/4" VCO   | 188.2 [7.41]                    | 156.0 [6.14]                    | 344.2 [13.55]                  | 312.0 [12.28]                  |  |  |  |
| 3.2MM UPG  | N/A                             | 150.3 [5.92]                    | N/A                            | N/A                            |  |  |  |
| ANSI/ISA 76.00.02  | N/A                             | Contact Factory                 | Not Ava                        | ailable                        |  |  |  |
| * OVERALL LENGTH FINGER TIGHT ** OVERALL LENGTH DIMENSION IS TO THE INTERNAL [INCH] TUBE LOCATING SHOULDER |                                 |                                 |                                |                                |  |  |  |

Figure 4 Lay-In Dimensions Integral and Remote Valves

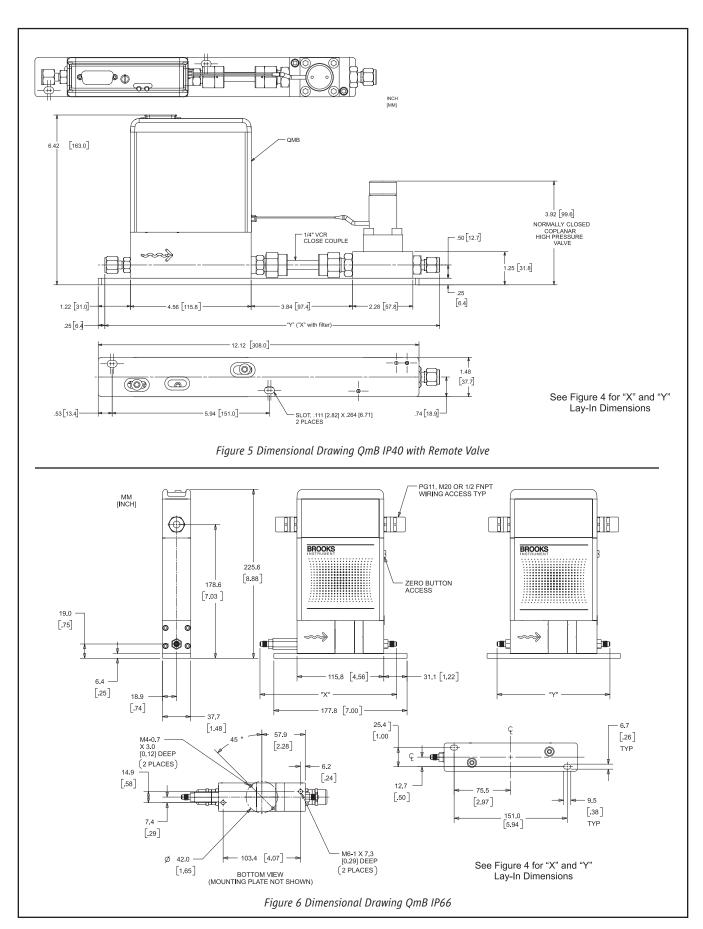

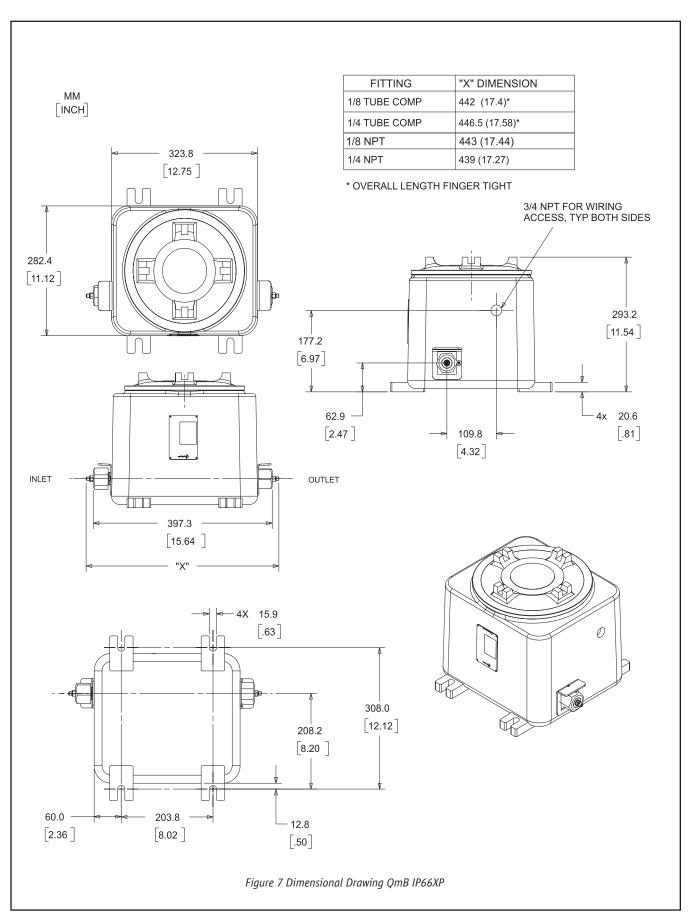

| Code    | Description                          | Code Option  | Option Descript               | ion              |                          |                      |
|---------|--------------------------------------|--------------|-------------------------------|------------------|--------------------------|----------------------|
|         |                                      |              |                               |                  |                          |                      |
| 1.      | Base Model Code                      | QMBC<br>QMBM | flow controller<br>flow meter |                  |                          |                      |
|         |                                      | QIVIDIVI     | now meter                     |                  |                          |                      |
| II.     | Tube Size                            |              | meter nominal                 | lflow            |                          | r nominal flow       |
|         |                                      |              | liqud                         | gas              | liquid                   | gas                  |
|         |                                      | 2            | 190 grams/hr                  | 1432 sccr        | ,                        | 1051 sccm            |
|         |                                      | 3            | 1.00 kg/hr                    | 5.595 slpr       |                          | 2.96 slpm            |
|         |                                      | 4            | 13.5 kg/hr                    | 53.12 slpr       | m 7.97 kg/hr             | 24.79 slpm           |
| III.    | Fluid Type                           | G            | gas                           | Note: sele       | ct primary fluid type. U | Iser can switch from |
|         |                                      | L            | liquid                        | liquid to g      | as and vice-versa. Reze  | eroing is required.  |
| IV.     | Pressure Transducer                  | 1            | no transducer                 |                  |                          |                      |
| IV.     | riessure iransuucei                  | 1            |                               |                  |                          |                      |
| V.      | Valve Type                           | Α            | no valve (prod                |                  |                          |                      |
|         |                                      | В            | normally close                |                  |                          |                      |
|         |                                      | C            | remote normal                 | lly closed high  | n pressure               |                      |
| VI.     | Accuracy                             | 2            | standard 0.2%                 | of rate          | liquid & stainless ste   | el                   |
|         | ·                                    | 3            | optional 0.5%                 | of rate          | liquid & stainless ste   | el                   |
|         |                                      | 3            | standard 0.5%                 |                  | gas or Hastelloy         |                      |
|         |                                      | 4            | optional 1.0%                 | of rate          | gas or Hastelloy         |                      |
| VII.    | Enclosure                            |              | Туре                          | Area (           | Classification           |                      |
| -11.    |                                      | А            | NEMA 1/ IP40                  | , iica (         |                          |                      |
|         |                                      | В            | NEMA 1/ IP40                  | Class            | 1 Div 2 Zone 2           |                      |
|         |                                      | С            | NEMA 4X/ IP66                 |                  | L DIV L LONG L           |                      |
|         |                                      | D            | NEMA 4X/ IP66                 |                  | 1 Div 2 Zone 2           |                      |
|         |                                      | E            | NEMA 4X/ IP66                 | SXP Div 1        | Zone 1                   |                      |
| 1/111   | Surface Finish                       | 1            | standard surfa                | aa finiah /22 .  | ۸)                       |                      |
| VIII.   | Surface Fillish                      | 1            | standard surfa                | ce iinish (32 i  | A)                       |                      |
| IX.     | Sensor Tube Material                 | Α            | stainless steel               | 316L             |                          |                      |
|         |                                      | В            | Alloy C-22 (tub               | oes only)        |                          |                      |
| X.      | Maximum Pressure Rating              | 1            | 35 bar or 500                 | nci              |                          |                      |
| Λ.      | Maximum Fressure Ruting              | 2            | 100 bar or 150                |                  |                          |                      |
|         |                                      | 3            | 300 bar or 450                |                  | tube material - Alloy    | C-22 (meter)         |
| VI      | Manipulation Terror continue Detical | Δ.           | (F.D C/14)                    | 0 D F\           | •                        |                      |
| XI.     | Maximum Temperature Rating           | А            | 65 Deg. C (14)                | 9 Deg F)         |                          |                      |
| XII.    | Process Connections                  | 1A           | standard body                 | connections 5    | 5/16" -24 UNF            |                      |
|         |                                      | 1B           | 1/16" tube cor                |                  |                          |                      |
|         |                                      | 1C           | 1/4" tube com                 |                  |                          |                      |
|         |                                      | 1D           | 1/8" tube com                 |                  |                          |                      |
|         |                                      | 1G           | 6mm tube com<br>1/8" NPT      | ipression fittii | ngs                      |                      |
|         |                                      | 1]<br>1K     | 1/8 NPT<br>1/4" NPT           |                  |                          |                      |
|         |                                      | 1L           | 1/4" VCR                      |                  |                          |                      |
|         |                                      | 1M           | 1/4" VCR                      |                  |                          |                      |
|         |                                      | 1P           | 1/4" VCO                      |                  |                          |                      |
|         |                                      | 1Y           | downport ANS                  | I/ISA - 76.00.0  | 02                       |                      |
|         |                                      | 2A           | 3.2mm UPG                     |                  |                          |                      |
| XIII    | Electrical I/O - Communications      |              | Primary Outpu                 | t                | Secondary Output         |                      |
| 74111   |                                      | А            | 0-5 Vdc                       | -                | 4-20 mA                  |                      |
|         |                                      | В            | 4-20 mA                       |                  | 4-20 mA                  |                      |
|         |                                      | C            | 0-5 Vdc                       |                  | 0-5 Vdc                  |                      |
|         |                                      | Н            | HART/4-20mA                   |                  | HART/4-20mA              |                      |
| XIV.    | Electrical Connection                | 1            | 15 pin D-type Enclosur        | e NFMA 1/ IP/    | 10                       |                      |
| 7 (1 V. |                                      | 3            | PG11 cable gland              |                  | NEMA 4X/ IP66            |                      |
|         |                                      | 4            | 1/2" FNPT conduit             |                  | NEMA 4X/ IP66            |                      |
|         |                                      | 6            | M20 FNPT conduit              |                  | NEMA 4X/ IP66            |                      |
|         |                                      | 8            | 3/4" FNPT conduit             | Enclosure        | NEMA 4X/ IP66XP          |                      |
| XV.     | Seals                                |              | Sensor                        | Valve Stem       | Fitting                  | Orifice Seal         |
| 7,00    |                                      | Α            | Viton                         | Viton            | Viton                    | Stainless Steel      |
|         |                                      | В            | Buna                          | Buna             | Buna                     | Stainless Steel      |
|         |                                      | C            | Kalrez 4079                   | Kalrez 4079      | Kalrez 4079              | Stainless Steel      |
|         |                                      | D            |                               | Kalrez 6375      | Kalrez 6375              | Stainless Steel      |
|         |                                      | E            | EPDM                          | EPDM             | EPDM                     | Stainless Steel      |
|         |                                      | F            | Nickel                        | Nickel           | Viton                    | Stainless Steel      |
|         |                                      | G            | Nickel                        | Nickel           | Buna                     | Stainless Steel      |

| Code Description              | Code Option | Option Desc        | ription   |                      |                     |  |  |  |  |  |
|-------------------------------|-------------|--------------------|---|----------------------|---------------------|--|--|--|--|--|
| XV. Seals (continued)         |             | Sensor             | Valve Stem  | Fitting              | Orifice Seal        |  |  |  |  |  |
|                               | Н           | Nickel             | Nickel  | Kalrez               | Stainless Steel     |  |  |  |  |  |
|                               | ]           | Nickel             | Nickel  | EPDM                 | Stainless Steel     |  |  |  |  |  |
|                               | K           | Nickel             | Nickel  | Nickel               | Stainless Steel     |  |  |  |  |  |
| XVI. Valve Seat Material      | 1           | none               |   | (meter)              |                     |  |  |  |  |  |
|                               | 7           | material 17-7P     | H Stainless Steel   | (controller)         |                     |  |  |  |  |  |
| XVII. Special Processing      | Α           | none               |   |                      |                     |  |  |  |  |  |
|                               | В           | certified materi   | al 2.2 EN 10204   |                      |                     |  |  |  |  |  |
|                               | С           | certified materi   | al 3.1 EN 10204   |                      |                     |  |  |  |  |  |
|                               | D           | cleaning for oxy   | cleaning for oxygen service   |                      |                     |  |  |  |  |  |
|                               | E           | cleaning for ox    | cleaning for oxygen service + certified material 2.2 EN 10204                                   |                      |                     |  |  |  |  |  |
|                               | F           | cleaning for ox    | cleaning for oxygen service + certified material 3.1 EN 10204                                   |                      |                     |  |  |  |  |  |
| XVIII. Quality Certifications | 1           | none               |   |                      |                     |  |  |  |  |  |
| ·                             | 2           | calibration cert   | calibration certificate traceble to NIST calibration measurement capability certificate (NVLAP) |                      |                     |  |  |  |  |  |
|                               | 3           | calibration mea    |   |                      |                     |  |  |  |  |  |
|                               | 4           |                    | certificate of conformance  |                      |                     |  |  |  |  |  |
|                               | 5           | calibration cert   | calibration certificate traceble to NIST + certificate of conformance                           |                      |                     |  |  |  |  |  |
|                               | 6           | calibration mea    | surement capability o   | ertificate + certifi | cate of conformance |  |  |  |  |  |
| XIX. Inline Filter            | Α           | none (             | metal seal or downpo  | rt)                  |                     |  |  |  |  |  |
|                               | В           | inline filter cart | tridge filter, 10 micror  | n (recommended       | for QMBC2)          |  |  |  |  |  |
|                               | C           | inline filter cart | tridge filter, 20 micror  | า                    |                     |  |  |  |  |  |
|                               | D           | inline filter cart | tridge filter, 30 micror  | า                    |                     |  |  |  |  |  |
|                               | E           | inline filter cart | tridge filter, 40 micro   | า                    |                     |  |  |  |  |  |
|                               | F           | inline filter cart | tridge filter, 1 micron   | (recommended for     | or QMBC2)           |  |  |  |  |  |
| XX. OEM Code                  | Α           | Brooks             |   |                      |                     |  |  |  |  |  |
|                               | N           | no logo            |   |                      |                     |  |  |  |  |  |

Sample Model Code

| Jan.ptc . |   |     |    |   |    |     |      |    |   |    |     |      |     |    |     |      |       |     |    |
|-----------|---|-----|----|---|----|-----|------|----|---|----|-----|------|-----|----|-----|------|-------|-----|----|
| _         | П | III | IV | ٧ | VI | VII | VIII | IX | Х | XI | XII | XIII | XIV | XV | XVI | XVII | XVIII | XIX | XX |
| QMBC      | 2 | G   | 1  | Α | 2  | Α   | 1    | Α  | 1 | Α  | 1A  | Α    | 1   | Α  | 1   | Α    | 1     | Α   | Α  |

Request a Quote

## Service and Support

Brooks is committed to assuring all of our customers receive the ideal flow solution for their application, along with outstanding service and support to back it up. We operate first class repair facilities located around the world to provide rapid response and support. Each location utilizes primary standard calibration equipment to ensure accuracy and reliability for repairs and recalibration and is certified by our local Weights and Measures Authorities and traceable to the relevant International Standards.

Visit www.BrooksInstrument.com to locate the service location nearest to you.

### START-UP SERVICE AND IN-SITU CALIBRATION

Brooks Instrument can provide start-up service prior to operation when required. For some process applications, where ISO-9001 Quality Certification is important, it is mandatory to verify and/or (re)calibrate the products periodically. In many cases this service can be provided under in-situ conditions, and the results will be traceable to the relevant international quality standards.

### CUSTOMER SEMINARS AND TRAINING

Brooks Instrument can provide customer seminars and dedicated training to engineers, end users, and maintenance persons. *Please contact your nearest sales representative for more details.* Due to Brooks Instrument's commitment to continuous improvement of our products, all specifications are subject to change without notice.

| TRADEMARKS                         |                                  |
|------------------------------------|----------------------------------|
| Brooks                             | Brooks Instrument, LLC           |
| All other trademarks are the prope | erty of their respective owners. |
|                                    |                                  |



DS-CM-QmB-eng/2021-09

### Your exclusive contact Brooks Instrument in France and Switzerland:

### Serv'Instrumentation

Z.I Broteau Nord 69540 Irigny - France Tél: +33 (0)4 78 51 47 50 Fax: +33 (0)4 78 51 59 96

Email: e-serv@servinstrumentation.fr Web: www.servinstrumentation.fr

Global Headquarters

Brooks Instrument 407 West Vine Street Hatfield, PA 19440-0903 USA Toll-Free (USA): 888-554-FLOW T: 215-362-3500

BrooksAM@BrooksInstrument.com

A list of all Brooks Instrument locations and contact details can be found at www.BrooksInstrument.com

©Copyright 2021 Brooks Instrument, LLC All rights reserved. Printed in U.S.A.

